

X-Ray Phase Nano-tomography by FZP-based X-Ray Microscopy Combined with Talbot Interferometry

Yanlin Wu^{1*}, Hidekazu Takano², Karol Vegso², Masato Hoshino², Koichi Matsuo³, Atsushi Momose^{1,2}

¹. Institute of Multidisciplinary Research for Advanced Materials, Tohoku University, Sendai, Japan.

². Japan Synchrotron Radiation Research Institute, Sayo, Japan.

³. Keio University School of Medicine, Tokyo, Japan.

*yanlin.wu.a1@tohoku.ac.jp

A 100-fold full-field X-ray microscope using a Fresnel zone plate (FZP) in combination with a Talbot interferometer for phase tomography was constructed at beamline 37XU, SPring-8 to visualize the morphology of mouse bone specimens with a sub-micron spatial resolution and keeping with 300 μm wide-field of view [1]. However, there was a problem that bone specimens shrunk occasionally due to synchrotron radiation irradiation during CT scans. In this work, a higher-efficiency FZP for 9 keV X-rays has been employed to observe bone samples having soft tissue structures with reduced radiation damage.

In this work, we constructed a 74.1-fold X-ray microscope with a FZP (ANT HZP-500 μm -100nm) of a diameter of 500 μm and a diffraction efficiency of 30.2% at 9 keV in combination with a Talbot interferometer (see Table 1) which was constructed at beamline 37XU as well. The Talbot interferometer consisting of a $\pi/2$ phase grating 2.39 μm in pitch and an absorption grating 2.4 μm in pitch was set in front of the image detector whose effective pixel size was 13.65 μm . Phase tomography was performed using the continuous fringe-scanning method [2].

By evaluation, the diffraction efficiency of the new FZP performed almost as designed; that is, the total radiation dosage to bone specimens has been reduced by four times than the previous experiment [1] with total exposure time of 0.5 hours. Figure 1 shows a cross-sectional phase tomogram of bone specimen (malleus of mouse, 14 days after birth) obtained in the previous experiment. The shrinkage of bone specimen was observed as motion artefacts, as indicated by yellow arrows especially at soft tissues inside the bone. In contrast, the soft tissue and bone has been clearly observed in this study without motion artefacts, as shown in Figure 2.

In conclusion, we have improved the image quality of phase tomograms by using a FZP of a higher diffraction efficiency and a large diameter for the X-ray microscope combined with a Talbot interferometer. It is expected that the presented approach for X-ray phase nano-tomography is effective for various applications including biological studies [3].

References:

[1]. A. Momose *et al*, SPIE Proc. **10391** (2017) 103910Y.

[2]. S. Kibayashi *et al*, AIP Conf. Proc., **1466** (2012), 261.

[3]. The experiments were performed in project 2016B1147, 2017A1288, 2017B1361 at BL37XU SPring-8, Japan. This study was financially supported by the ETATO-Momose quantum beam phase imaging project (Grant Number JPMJER1403) of Japan Science and Technology Agency (JST), Japan.

Table 1. Parameters of ATN/FZP--SiC86/416 (NTT Advanced Technology Corporation [NTT-AT], Japan) FZP used in ref. [1] and HZP (Hard X-ray Fresnel zone plates) -500 μ m-100nm FZP (Applied Nanotools Inc [ANT], Canada) employed in this study.

Parameter	ATN/FZP--SiC86/416	HZP-500 μ m-100nm
Diameter	416 μ m	500 μ m
Outermost zone width	86 nm	100 nm
Zone thickness	700 nm (Ta)	1469 nm (Au)
Membrane thickness	2 μ m (SiC)	100 nm (SiN)
Focal length @9 keV	261 mm	365 mm
1st order diffraction efficiency @9 keV	8.6%	30.2%
0st order diffraction efficiency @9 keV	72.2%	7.6%

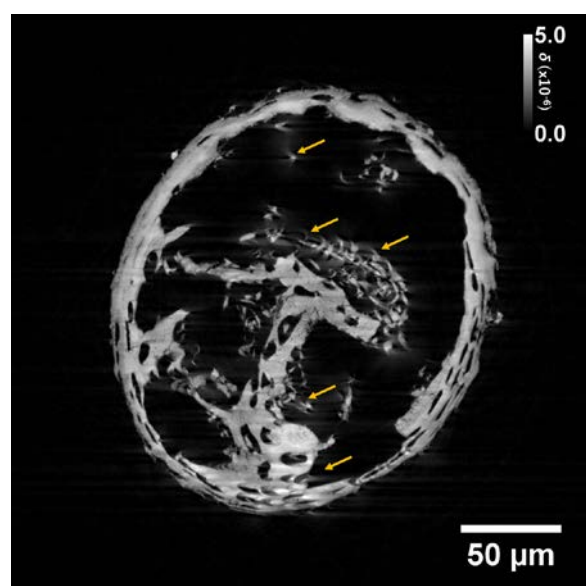


Figure 1. A phase tomogram (cross-section) of a bone specimen (malleus of mouse) obtained by the previous [1].

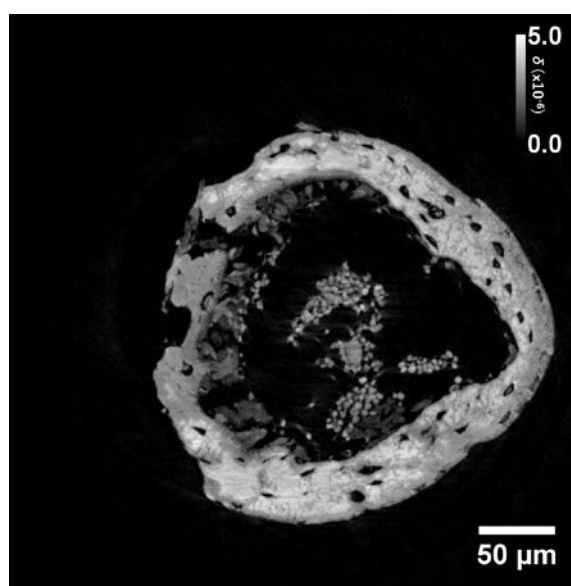


Figure 2. A phase tomogram (cross-section) of a bone specimen obtained in this work.