

PREHOSPITAL and DISASTER MEDICINE

Médecine Pré-Hospitalière et Médecine de Catastrophe

Volume 6, Number 3

July–September 1991

Original Research

On-Scene Time with Refusal of Treatment or Transport
Hepatitis B Serologic Markers in EMS Personnel
The Impact of Standing Orders
Criteria to Treat and Release Patients
Sudden Death in Young Patients
Peer-Review Quality Assurance

Brief Report

The On-Scene Physician
The Prehospital Use of Albuterol Inhalation Treatments

We Believe

Cardiopulmonary Arrest in Rural Areas

Collective Review

Urban Heavy Rescue

Venue

National Association of Emergency Medical Services Physicians
Seventh Annual Conference Venue and Abstracts
June 12–14, 1991

The Official Journal of the
National Association of EMS Physicians and the
World Association for Emergency and Disaster Medicine
in association with the
Acute Care Foundation and the
National Association of State EMS Directors

Marquette announces a defibrillator that thinks



The new Responder™ 1500 is the next best thing to having a cardiologist at your side. The 1500 is a full-featured defibrillator with the added capability of on-the-spot computer-analyzed 12-lead ECGs. It is a complete defibrillator and a computer-enhanced electrocardiograph in one lightweight package.

The Responder 1500 uses Marquette's proven 12SL analysis program to collect data from all 12 leads simultaneously and to perform a full analysis of morphology and rhythm in just 15 seconds. The report, which is printed instantly, can also be transmitted by cellular or conventional telephone to a cardiologist for overreading and verification. The 1500 makes pre-hospital thrombolytic therapy a real possibility.

The 12SL program is used worldwide. The sensitivity and specificity with which it recognizes acute myocardial infarction is based on a data base of 20 million ECGs. Breakthroughs in computer miniaturization technology permit this powerful and accurate program to be included in the 1500.

The 1500 also features full-disclosure digital ECG recording for unprecedented medical control capabilities. All field data can be reviewed, analyzed and printed, or stored for later review. Other, optional features include external pacing (demand or non-demand) and an arrhythmia advisory system.

For more information about the versatile Responder 1500, contact your Marquette representative or call us at 1-800-558-5120, ext. 3000.



Marquette Emergency Care Division
U. S. A.: 8200 W. Tower Ave. • Milwaukee, Wisconsin 53223
Tel. (414) 355-5000 • TLX 297991 MEI UR • FAX (414) 357-0415
Europe: 15, rue Rougemont • 75009 Paris, France
Tel. (33) (1) 42.46.00.19 • FAX (33) (1) 48.01.04.41
Asia/Pacific: 181 Johnston Rd. • Suite 1010 • Wanchai,
Hong Kong • Tel. (852) 8381398 • FAX (852) 8381507

M01047E1


Editor's Corner: Resurrection Isn't Everything	287
 Original Research	
Paramedic On-Scene Time for Patients Initially Refusing Treatment or Transport	293
<i>John M. Heiser, MD, Robert L. Norton, MD, Keith W. Neely, EMT-P, MPA, Joe Acker, Jerris R. Hedges, MD</i>	
A Meta-Analysis of Hepatitis B Serologic Marker Prevalence in EMS Personnel	299
<i>James Menegazzi, PhD</i>	
The Impact of Standing Orders on Medication and Skill Selection, Paramedic Assessment, and Hospital Outcome: A Follow-up Report	303
<i>James E. Pointer, MD, Michael Osur, EMT-P, Colleen Campbell, Ben H. Mathews, MPH, Chet McCall, PhD</i>	
Development and Evaluation of Criteria Allowing Paramedics to Treat and Release Patients Presenting with Hypoglycemia: A Retrospective Study	309
<i>Randy H. Thompson, EMT-P, Robert W. Wolford, MD</i>	
Non-Traumatic Prehospital Sudden Death in Young Patients: An Urban EMS Experience	315
<i>Larry D. Weiss, MD, Stanley Janasiewicz, MD, Joshua A. Perper, MD, Vincent P. Verdile, MD, Donald M. Yealy, MD, James J. Menegazzi, PhD</i>	
A Paramedic Peer-Review Quality Assurance Audit	321
<i>Robert A. Swor DO, FACEP, Joseph J. Bocka MD, Ronald F. Maio DO, FACEP</i>	
 Brief Reports	
The Prehospital Use of Albuterol Inhalation Treatments	327
<i>Eric A. Vonderohe, MD, James H. Jones, MD, FACEP, Roland B. McGrath, MD, Leon H. Bell, EMT-P</i>	
Paramedic Perceptions of the On-Scene Physician	331
<i>Larry B. Mellick, MD, Helen Yurong, MS, MSN, NREMT-P, Kathey Haley, RN, Douglas Ferguson, MD</i>	
 We Believe	
Clinical Guidelines for Delayed/Prolonged Transport: I. Cardiorespiratory Arrest	335
<i>Rural Affairs Committee, National Association of Emergency Medical Services Physicians Peter Goth, MD, George Garnett, MD</i>	
 Collective Review	
Medical Aspects of Urban Heavy Rescue	341
<i>John D. Moede, Paramedic III</i>	
 Seventh Annual Conference of the NAEMSP (Orlando, Florida, USA)	
Faculty	364
Program	365
Oral Presentations	370
Poster Presentations	384
<hr/>	
Forum	349
Calendar	352

Rtiti

RUSTRONICS, INC.


OUR BUSINESS IS INNOVATION. OUR FOCUS IS EMS.

MAGNUM™

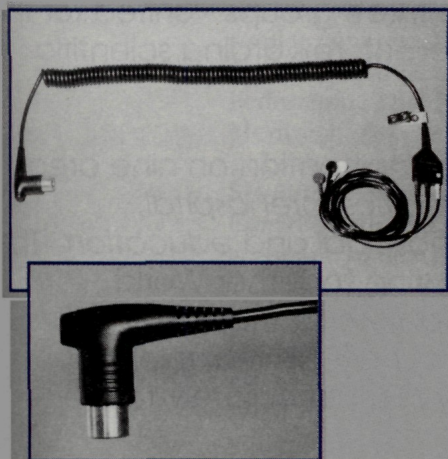


The MAGNUM™ series of heavy-duty EKG cables are specifically designed to meet the demanding needs of pre-hospital medicine, with all stress points reinforced with strain reliefs. The right-angle plug orients these cables in the right direction as soon as they are plugged in. They are offered in both the revolutionary *Coil-Cord* configuration with heavy-duty shielding and in traditional straight-cable style. MAGNUM™ series cables are designed to last and are covered by a one-year warranty.

Godfrey-LOCK™

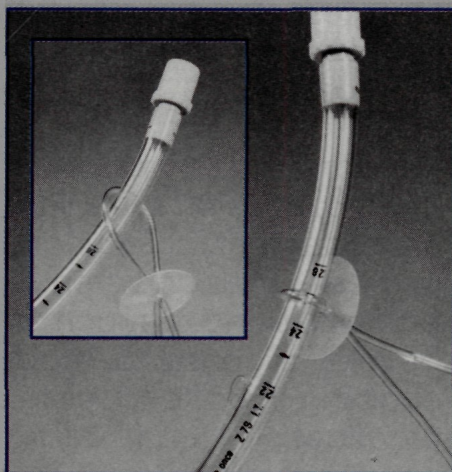

The Godfrey-LOCK™ is an extremely simple, low-cost fixation device that *securely* immobilizes an endotracheal tube, even in the presence of vomitus, blood and other secretions. The G-LOCK™ was developed to alleviate the field technique of cutting IV tubing and tying the endotracheal tube in place, but the G-LOCK™ is *easier* to use and *much* more economical than destroying an IV set. Limited quantities of *free* samples are available.

L.A.P. 5™

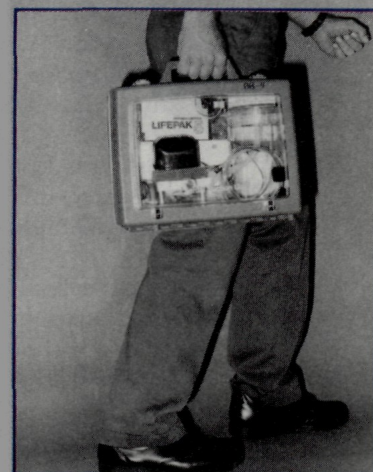

The Laerdal Alternative Power 5™ system enables Laerdal suction units to be powered by LIFEPAK 5-type monitor defibrillator batteries. The LAP 5™ system creates battery compatibility between the suction unit and monitor/defibrillator equipment, allowing spare battery availability on the scene. It cuts battery replacement costs by 50 percent and charge time by 75 percent. The unit provides more than 45 minutes of continuous working-strength suction, clearing 1000ml of water in 5.3 seconds. Best of all, it provides a *remote switch* for one-handed operation. The LAP-5™ system breathes new life into your Laerdal suction units for a fraction of the cost of new suction equipment.

1587 S. Niemeyer Circle • Port St. Lucie, FL 34952 • (407) 337-0333

TOLL FREE 1-800-326-0278

LIFEPAK 5™ and Laerdal Suction Unit are trademarks of Physio-Control and Laerdal Medical Corp. respectively and are not affiliated with Rustronics, Inc.

<https://doi.org/10.1017/S1049023X00038681> Published online by Cambridge University Press

PREHOSPITAL and DISASTER MEDICINE

Médecine Pré-Hospitalière et Médecine de Catastrophe

THE OFFICIAL JOURNAL OF THE WORLD ASSOCIATION FOR EMERGENCY AND DISASTER MEDICINE (WAEDM)

THE NATIONAL ASSOCIATION OF EMERGENCY MEDICAL SERVICES PHYSICIANS (NAEMSP)

IN ASSOCIATION WITH THE ACUTE CARE FOUNDATION AND

THE NATIONAL ASSOCIATION OF STATE EMERGENCY MEDICAL SERVICES DIRECTORS (NASEMSD)

EDITOR

Marvin L. Birnbaum, MD, PhD
University of Wisconsin-Madison
Madison, Wisconsin, USA

ASSOCIATE EDITORS

Michael Copass, MD
Harbor View Medical Center
University of Washington
Seattle, Washington, USA

Michael Gunderson, REMT-P
Pinellas County EMS System
Tampa, Florida, USA

Steven Rottman, MD
UCLA Hospitals and Clinics
Los Angeles, California, USA

Martin Silverstein, MD
Uniformed Services Univ. of the
Health Sciences
Bethesda, Maryland, USA

PAST EDITORS

R Adams Cowley, MD
Charles Mac Mathias
National Study Center
Baltimore, Maryland, USA
(JWAEDM 1986-87)

Peter Safar, MD
University of Pittsburgh
Pittsburgh, Pennsylvania, USA
(JWAEDM 1981-85)

Michael Gunderson, REMT-P
Pinellas County EMS System
Tampa, Florida, USA
(JPM 1987-88)

CONSULTING EDITORS

Peter Safar, MD
University of Pittsburgh
Pittsburgh, Pennsylvania, USA

Ronald Stewart, MD
Victoria Hospital
Halifax, Nova Scotia, Canada

Jakov Adler, MD
Shaare Zedec Medical Center
Jerusalem, Israel

Fritz Ahnefeld, MD
University of Ulm
Ulm, Germany

Paul B. Anderson
Idaho Office of EMS
Boise, Idaho, USA

Jack Ayres, JD, REMT-P
University of Texas Health Science Center
Dallas, Texas, USA

Peter Baskett, MD
Frenchay Hospital
Bristol, UK

Jeff Clawson, MD
Salt Lake City Fire Department
Salt Lake City, Utah, USA

Richard Cummins, MD
University of Washington
Seattle, Washington, USA

Craig DeAtley, PA-C
Geo. Washington Univ. Med. Ctr.
Washington, DC, USA

Eelco Dykstra, MD
Center for International EMS
Wiesbaden, Germany

Morgan Fahey, MD, OBE
Shirley Medical Centre
Christchurch, New Zealand

Judith Fisher, MD
British Association for Immediate Care
London, UK

Malcolm Fisher, MD
Royal North Shore Hospital
Sydney, Australia

George Garnett, MD
Soldotna, Alaska, USA

S. William A. Gunn, MD
European Centre for Disaster Medicine
Medical Society of the WHO
Geneva, Switzerland

Mark S. Johnson
Alaska Dept. Public Health
Juneau, Alaska, USA

Michael King, REMT
Acute Care Foundation
Tampa, Florida, USA

John C. Lane, MD
University of Campinas Medical Center
Sao Paulo, Brazil

Baxter Larmon, EMT-P
UCLA Medical Center
Los Angeles, California, USA

Susan D. McHenry
Virginia Dept. of Health
Richmond, Virginia, USA

Norman E. McSwain, Jr., MD
Tulane University Medical Center
New Orleans, Louisiana, USA

EDITORIAL BOARD

Sergio Magalini, MD
Universita Cattolica del Sacro Cuore
Rome, Italy

Ronald F. Maio, DO
University of Michigan Medical Center
Ann Arbor, Michigan, USA

Kimball Maul, MD
University of Tennessee
Knoxville, Tennessee, USA

Michael Moles, MD
Prince Philip Hospital
Hong Kong University
Hong Kong

Eric Noji, MD
United States Centers for Disease Control
Atlanta, Georgia, USA

Judy Olson, BSN
University of Wisconsin-Madison
Madison, Wisconsin, USA

James O. Page, JD
Emergency Care Information Center
Carlsbad, California, USA

Paul Paris, MD
University of Pittsburgh
Pittsburgh, Pennsylvania, USA

Jiri Pokorny, MD, DrSc.
Post-Graduate Medical School
Prague, Czechoslovakia

Ameen I. Ramzy, MD
University of Maryland
Baltimore, Maryland, USA

Lawrence W. Rose, MD
Bethesda, Maryland, USA

Sandra M. Schneider, MD
University of Pittsburgh
Pittsburgh, Pennsylvania, USA

Victor Semenov, MD
Reanimatology Institute
Academy of Medical Sciences
Moscow, USSR

Carol J. Shanaberger, JD
Denver Colorado, USA

Shao Xiaohong, MD
Chinese Academy of Medical Sciences
Peking Union Medical College
Beijing, PRC

John Shea, MD
Loyola University Medical Center
Maywood, Illinois, USA

Kenneth Stults, PA-C
Harris Methodist Fort Worth
Fort Worth, Texas, USA

Takashi Ukai, MD
Senri Critical Care Medical Center
Osaka, Japan

Connie Walleck, RN, MS
Health Science Center SUNY-Syracuse
Syracuse, New York, USA

Publication and Production Editor

Roland Tracy Will II
School of Medicine
University of Wisconsin-Madison, USA

Elizabeth Chapin
Editorial Assistant

Advertising, Production and Subscription

Jems Communications

James O. Page, **Publisher**
Keith Griffiths, **Executive Editor**
Dana Jarvis Bies, **Director of Production**
Gail M. Williams, **Graphics Specialist**
Janene Long, **Production Coordinator**
MaryBeth Locastro, **Advertising Director**
Lisa J. Cota, **Account Executive**
Marte Reavis, **Account Executive**
Jay Hillis, **Circulation/Marketing Director**
David B. Forman, **Marketing Coordinator**
Kevin Petrie, **Fulfillment Manager**

Prehospital and Disaster Medicine (ISSN 1049-023X) is published quarterly in the months of December, March, June, and September by Jems Communications, 1947 Camino Vida Roble, Carlsbad, CA 92008-6513, USA; (619) 431-9797. *Prehospital and Disaster Medicine* incorporates the *Journal of the World Association for Emergency and Disaster Medicine* and the *Journal of Prehospital Medicine*.

Editorial Information: Submit manuscripts and editorial inquiries to: Marvin L. Birnbaum, MD, Editor, *Prehospital and Disaster Medicine*, 1552 University Avenue, Room 434, Madison, WI 53705, USA; (608) 263-7094, (608) 263-2069, Fax (608) 263-2069.

Subscription Information: One year (four issues)—Institutions: (U.S.) \$78; Individuals: \$48; Residents/In Training: \$35; Paramedic, Nurse, EMT: \$35. Canadian subscribers must add \$10 per year, and international subscribers add (U.S.) \$20 per year for postage. Claims of non-receipt or damaged issues must be filed within three months of cover date.

Advertising Information: Contact Jems Communications, P.O. Box 2789, Carlsbad, CA 92018; (619) 431-9797; Fax (619) 431-8176

Abstracts: Abstracts available in the National Association of EMS Physicians Electronic Database and the Emergency Care Information Center (ECIC).

Copyright © 1991 by the National Association of Emergency Medical Services Physicians (USA), World Association for Emergency and Disaster Medicine, and the Acute Care Foundation.

Postmaster (USA): Return form 3579 to Jems Communications, P.O. Box 2789, Carlsbad, CA 92018.

Second Class Postage pending at Carlsbad, CA 92008 and additional mailing offices.

Identification of CO₂ immediately following intubation is fast and simple with the MiniCAP™ III CO₂ detector.

Establish airways with confidence, not color change.

Using sophisticated infrared technology connected directly to the endotracheal tube, the MiniCAP III detects the presence and absence of CO₂ during the respiration cycle. A loss of respiration alarm is provided, adjustable from 5–60 seconds.

Unlike disposable chemical-type detectors, the MiniCAP III uses bright LEDs and an audible tone to indicate a complete respiratory cycle under any ambient light condition. The MiniCAP III also provides visual and audible alarms for loss of respiration, which chemical-type detectors can't provide.

Rugged and reliable, the battery-powered MiniCAP III CO₂ detector belongs with every intubation kit on crash carts or in ambulances. Don't settle for anything less.

For further details on the CO₂ detector you can use with confidence, call 1-800-672-4678, Ext. 8826.

MSA CATALYST RESEARCH

3706 Crondall Lane
Owings Mills, MD 21117
301/356-2400
Fax: 301/581-0346

